



AOD Central Fabrication
 12315 Judson Rd. #206
 San Antonio, TX 78233

SUPRAMALLEOLAR AFO

Patient _____ PO# _____ Diagnosis _____
 Clinic _____ Due Date (Rush Fee May Apply) _____
 Clinician _____ Height _____ Weight _____
 Phone _____ Age _____ Sex _____ Shoe Size _____

PATIENT ID		<small>INTERNAL USE - DO NOT FILL IN PATIENT ID</small>
-------------------	--	---

Step 1: Device Type

L B R SMO with Plantarflexion Stop	L B R Standard SMO
Alternate Footplate Plastic Lengths* <input type="checkbox"/> Proximal to Metatarsal Heads <input type="checkbox"/> Full Length  <input type="checkbox"/> EVA Footplate Padding (Full Length) <small>*Standard Plastic Length is to Sulcus</small>	Alternate Footplate Plastic Lengths* <input type="checkbox"/> Proximal to Metatarsal heads <input type="checkbox"/> Full Length  <input type="checkbox"/> EVA Footplate Padding (Full Length) <small>*Standard Plastic Length is to Sulcus</small>

Straps and pads included, but not shown above. Check back of form for material specifications. Plastic will be selected based on patient weight.


Step 2: Modifications and Additions

Primary Color or Transfer Pattern: Natural Black Blue Pink US Flag Forest Camo Other

ANKLE AND REARFOOT	ANKLE AND REARFOOT	MIDFOOT	FOREFOOT
L B R Do Not Change Ankle* Or Change to _____	L B R Medial Wedge Height or Angle _____	L B R Increase Arch Height	L B R Do Not Change* Or Change to _____
L B R Do Not Change Rearfoot* Or Change to _____	L B R Lateral Wedge Height or Angle _____	L B R Decrease Arch Height	L B R Metatarsal Pad Small Medium Large
	L B R Posterior Wedge Height or Angle _____	L B R Navicular Relief	L B R Toe Crest Pad
		L B R Cuboid Relief	

*Ankle, rearfoot, and forefoot correction to neutral is standard.

Step 3: Order Notes and Special Requests



(P) 210-657-8100
 (F) 210-657-8105


RECEIVED DATE	COMPLETED DATE

info@aodcfab.com

SUPRAMALLEOLAR AFO

Step 4: Measurements

Measurements are not necessary, but will improve the accuracy of the final product.

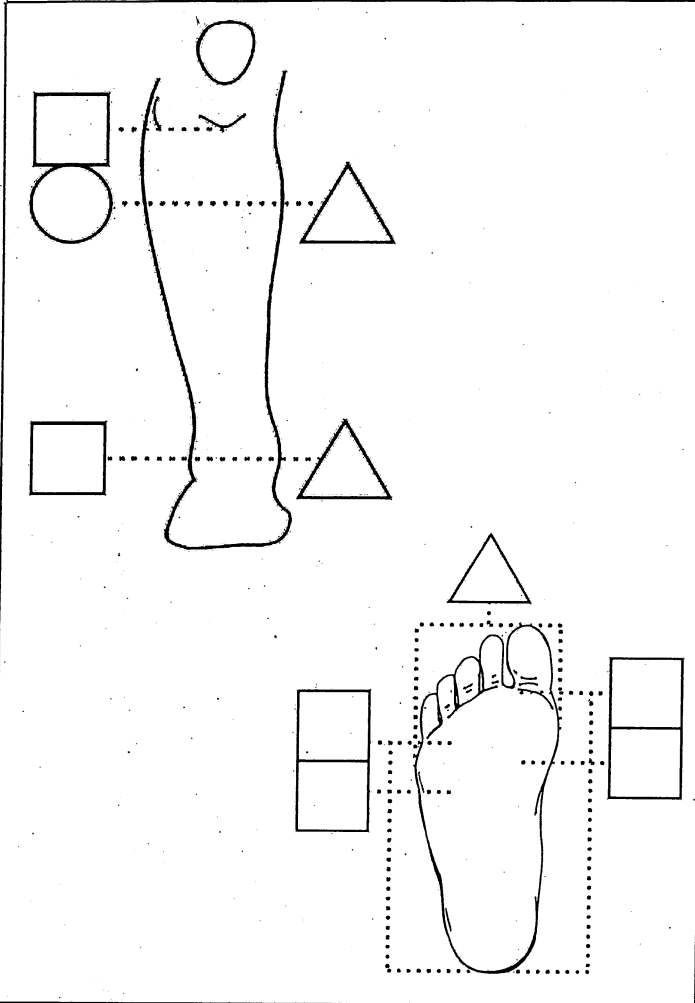

Material Specifications

Call with questions or for other material options.
Warranty information available at www.AODCFAB.com

SMO with Plantarflexion Stop

- Polypropylene Homopolymer Shell and Posting
- 35 Durometer EVA Padded Footplate *optional*
- 25 Durometer EVA Malleolar and Arch Padding
- 35 Durometer EVA Posterior Stop Padding

SMO

- Polypropylene Homopolymer Shell and Posting
- 35 Durometer EVA Padded Footplate *optional*
- 25 Durometer EVA Malleolar and Arch Padding

INTERNAL USE - DO NOT WRITE BELOW

CUSTOMER COMMUNICATIONS